

PEOPLE HAVE PRIORITY



synea FUSION

Instructions for use



CE
0297

Turbine handpieces with light

TG-98 L / TG-97 L / TG-98 LM / TG-97 LM

TG-98 L N / TG-97 L N / TG-98 L RM / TG-97 L RM

Turbine handpieces without light

TG-98 / TG-97

Contents

Symbols	4
in the Instructions for use	4
on the medical device / packaging.....	5
1. Introduction	6
2. Safety notes	9
3. Product description	14
Roto Quick coupling	14
<i>Multiflex</i> ^{®*} , <i>NSK</i> ^{®*} <i>connection</i>	15
Turbine with RM connection.....	16
4. Operation	17
Assembly / Removal	17
To change rotary instrument	21
Test run	22
5. Hygiene and maintenance	23
General notes	23

Limitations on processing.....	25
Initial treatment at the point of use.....	26
Manual cleaning.....	27
Automated cleaning and lubrication	32
Manual cleaning.....	33
Automated cleaning and disinfection.....	34
Drying	35
Inspection, Maintenance and Testing.....	36
Packaging.....	40
Sterilization	41
Storage.....	43
6. Servicing	44
7. W&H Accessories and spare parts	45
8. Technical data.....	46
9. Disposal	49
Explanation of warranty terms.....	50
Authorized W&H service partner	51



WARNING!
(risk of injury)



ATTENTION!
(to prevent
damage occurring)













General explanations,
without risk to
persons or objects



Do not dispose of with
domestic waste

Symbols

on the medical device / packaging

	CE marking with identification number of the Notified Body		DataMatrix Code for product information including UDI (Unique Device Identification)		Data structure in accordance with Health Industry Bar Code
	Catalogue number		Thermo washer disinfectable		Sterilizable up to the stated temperature
	Serial number		UL Component Recognition Mark indicates compliance with Canadian and U.S. requirements		
	Date of manufacture		Caution! According to Federal law, this medical device may only be sold by or on the order of a dentist, physician or any other medical practitioner licensed by the law of the State in which he or she practices and who intends to use or order the use of this medical device		

1. Introduction

Customer satisfaction has absolute priority in the W&H quality policy. This medical device has been developed, manufactured and subjected to final inspection according to legal regulations, quality and industry standards.

For your safety and the safety of your patients

Prior to initial use please read the Instructions for use. These explain how to use your medical device and guarantee a smooth and efficient operation.



Observe the safety notes.

Intended use

The dental turbine is intended for the following applications: Removal of decayed materials, cavities and crown cement, removal of fillings, finishing of tooth and restoration surfaces.



Misuse may damage the medical device and hence cause risks and hazards for patient, user and third parties.

Qualifications of the user

We have based our development and design of the medical device on the dentists, dental hygienists, dental employees (prophylaxis) and dental assistants target group

Production according to EU Directive

 The medical device meets the requirements of Directive 93/42/EEC.

0297

Responsibility of the manufacturer

The manufacturer can only accept responsibility for the safety, reliability and performance of the medical device when it is used in compliance with the following directions:

- > The medical device must be used in accordance with these Instructions for use.
- > Only the components approved by the manufacturer may be replaced (seal and water filter)
- > Modifications or repairs must only be undertaken by an authorized W&H service partner (see page 51).

Skilled application

The medical device is intended only for skilled application according to the intended use as well as in compliance with the valid health and safety at work regulations, the valid accident prevention regulations and in compliance with these Instructions for use.

The medical device should be prepared for use and maintained by staff who have been trained in procedures for infection control, personal safety and patient safety.

Improper use, (e.g., through poor hygiene and maintenance), non-compliance with our instructions or the use of accessories and spare parts which are not approved by W&H, invalidates all claims under warranty and any other claims.

2.Safety notes



- > Before using the medical device for the first time, store it at room temperature for 24 hours.
- > The operation of the medical device is permitted only on supply units which correspond to the standards IEC 60601-1 (EN 60601-1) and IEC 60601-1-2 (EN 60601-1-2).

The power supply unit for the dental unit must satisfy the following requirements to be guaranteed by the system assembler:

- > Double insulation for the highest expected supply voltage must be provided between the primary and secondary power circuits.
- > Double insulation for the highest expected secondary voltage must be provided between the secondary voltage and protective earth (PE).
- > The secondary circuits must be galvanically isolated from each other.
- > The secondary circuits must be protected against short-circuiting and overloading.
- > The leakage currents of the applied part must be kept.
- > The secondary voltage in operation must be limited to a maximum of 4,2 V AC or 6 V DC.



- > Use only the supply hoses as specified by EN ISO 9168
- > Always ensure the correct operating conditions and cooling function.
- > Always ensure that sufficient and adequate cooling is delivered and ensure adequate suction.
- > In case of coolant supply failure, the medical device must be stopped immediately.
- > Use only the filtered, oil-free and cooled air supplied by dental compressors for drive air
- > Check the medical device for damage and loose parts before each use (e.g. push-button).
- > Do not operate the medical device if it is damaged.
- > Perform a test run before each use.
- > Avoid overheating at the treatment site.
- > Do not use the medical device if there are soft tissue wounds in the mouth. The air pressure can cause septic substances to enter the tissue or trigger embolisms.
- > Do not lift the cheek or tongue with the medical device. Risk of burning due to the push-button heating up!



- > Run the rinse function for the dental unit once per day.
- > Do not use the medical device as a light probe.
- > Do not look directly into the LED.



TG-98 L, TG-98 L RM, TG-97 L, TG-97 L RM are not approved for operation in potentially explosive atmospheres.



Risks due to electromagnetic fields

TG-98 L, TG-98 L RM, TG-97 L, TG-97 L RM

The functionality of implantable systems, such as cardiac pacemakers and ICD (implantable cardioverter defibrillator) can be affected by electric, magnetic and electromagnetic fields.

- > Find out if patient and user have implanted systems before using the medical device and consider the application.
- > Weigh the risks and benefits.
- > Keep the medical device away from implanted systems.
- > Make appropriate emergency provisions and take immediate action on any signs of ill-health.
- > Symptoms such as raised heartbeat, irregular pulse and dizziness can be signs of a problem with a cardiac pacemaker or ICD (implantable cardioverter defibrillator).

Hygiene and maintenance prior to initial use




- > The medical device is sealed in PE film and not sterilized when delivered
- > The PE film and the packaging are non-sterilizable



- > Clean, disinfect and lubricate the medical device.
- > Sterilize the medical device and the nozzle cleaner.

3. Product description


Roto Quick coupling

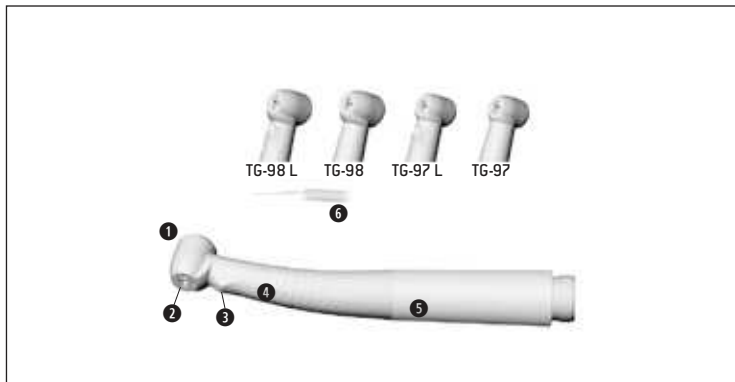

- ① Push-button
- ② Spray nozzles
- ③ LED
- ④ Grip profile
- ⑤ Sheath
- ⑥ Nozzle cleaner


3. Product description

Multiflex®, NSK®* connection*

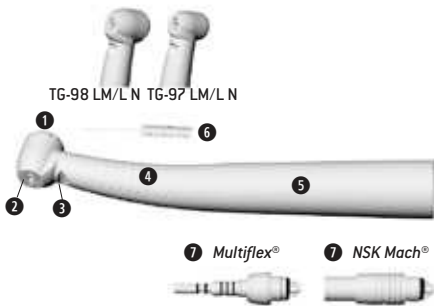


3. Product description

Turbine with RM connection

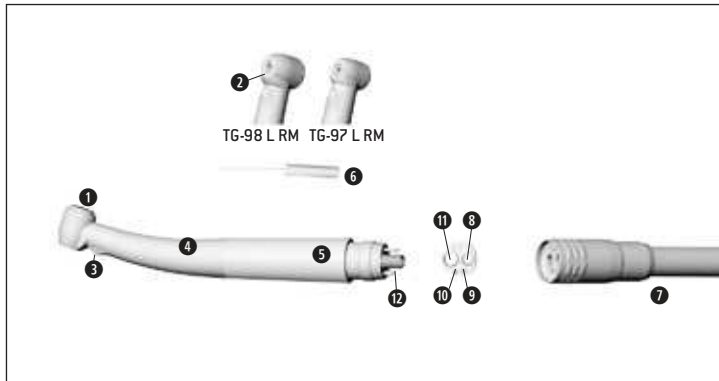

- 1 Push-button
- 2 Spray nozzles
- 3 LED
- 4 Grip profile
- 5 Sheath
- 6 Nozzle cleaner
- 7 Supply hose
- 8 Drive air
- 9 Coolant
- 10 Spray air
- 11 Exhaust air
- 12 Water filter with resuction stop

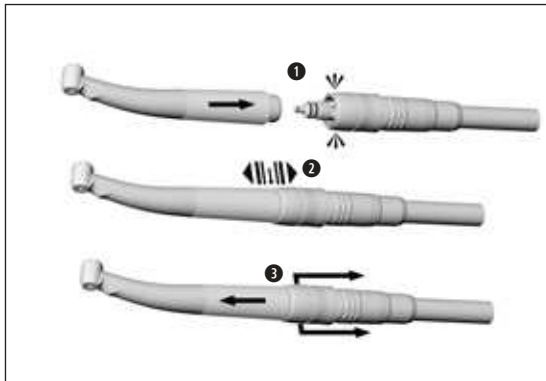

Roto Quick coupling



Do not assemble or remove the medical device during operation.

- 1** Push the medical device onto the Roto Quick coupling.



- 2** Verify full engagement.

- 3** Pull the retention sleeve of the Roto Quick coupling back and remove the medical device by pulling in an axial direction.

Multiflex[®], NSK Mach[®] connection




Do not assemble or remove the medical device during operation!

- > Attach the medical device to the Multiflex[®], NSK Mach[®] coupling as described by the coupling manufacturer.



> Verify full engagement.

- > Remove the **medical device from the Multiflex[®], NSK Mach[®]** coupling as described by the coupling manufacturer.

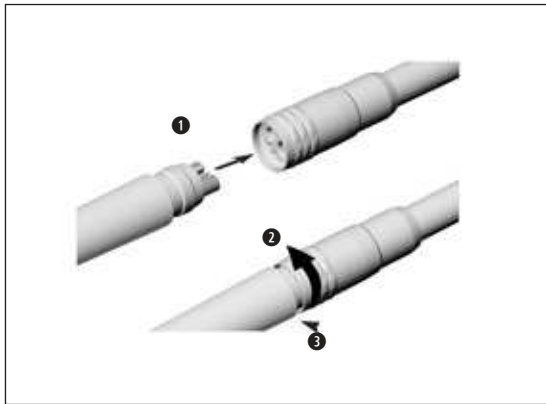

RM connection



Do not assemble or remove the medical device during operation!

- 1 Insert the medical device with RM connection into the apertures of the supply hose.
- 2 Firmly screw the union nut on.



3 Verify full engagement.
Check leak tightness.

- 4 Unscrew the union nut and remove the medical device from the supply hose.

Rotary instruments



- > Use only rotary instruments which are in perfect condition. Follow the operating instructions of the manufacturer
- > Insert the rotary instrument only when medical device is stationary.
- > Do not interfere with the running or slowing down of the rotary instrument.
- > Do not activate the push-button of the medical device during operation or slowing down. This leads to detachment of the rotary instrument resp. heating of the push-button (risk of injury).
- > Only use rotary instruments up to the maximum operating speed stipulated by the manufacturer.



To change rotary instrument

- 1 Insert the rotary instrument.
Activate push-button, at the same time insert the rotary instrument until back stop.



- 2 Verify full engagement.

- 3 Remove the rotary instrument by pushing the push-button.

Test run



Do not hold the medical device at eye level!

- > Insert the rotary instrument.
- > Start the medical device.



In the event of operating malfunctions (e.g., vibrations, unusual noise, overheating, coolant failure or leakage) **stop the medical device immediately** and contact an authorized W&H service partner.



Follow your local and national laws, directives, standards and guidelines for cleaning, disinfection and sterilization.



> Wear protective clothing, safety glasses, face mask and gloves



> Use only oil-free, filtered compressed air with a maximum operating pressure of 3 bar for manual drying.

Cleaning agents and disinfectants



- > Read the notes, follow the instructions and heed the warnings provided by the manufacturers of cleaning agents and/or disinfectants.
- > Use only detergents which are intended for cleaning and/or disinfecting medical devices made of metal and plastic.
- > It is imperative to comply with the concentrations and exposure times specified by the manufacturer of the disinfectant.
- > Use disinfectants which have been tested and found effective by the Verbund für Angewandte Hygiene e.V (VAH = Association for Applied Hygiene), the Österreichischen Gesellschaft für Hygiene, Mikrobiologie und Präventivmedizin (ÖGHMP = Austrian Society for Hygiene, Microbiology and Preventive Medicine), the Food and Drug Administration (FDA) and the U.S. Environmental Protection Agency (EPA).



The user is responsible for validating its process if the specified cleaning agents and disinfectants are not available.



The product lifetime and the medical device's ability to operate correctly are mainly determined by mechanical stress during use and chemical influences due to processing.

Send worn or damaged medical devices and/or medical devices with material changes to an authorized W&H service partner.



Processing cycles

> We recommend a regular service for the W&H medical device after 1,000 processing cycles or one year.



Clean and disinfect the medical device immediately after every treatment, to flush out liquid (e.g., blood, saliva etc.) and to prevent settling on the internal parts.g., blood, saliva etc.) and to prevent settling on the internal parts.

- > Operate the medical device for at least 10 seconds at idle speed.
- > Ensure that all outlets are rinsed out.



- > Wipe the entire surface of the instrument with disinfectant.
- > Remove the rotary instrument.
- > Remove the medical device.




Note that the disinfectant used during pre-treatment is only for personal protection and cannot replace the disinfectant step after cleaning.



Do not place the medical device in liquid disinfectant or in an ultrasonic bath!

- > Clean the medical device under running tap water (<35°C / 95°F).
- > Rinse and brush off all internal and external surfaces.
- > Move moving parts back and forth several times.
- > Remove any liquid residues using compressed air.

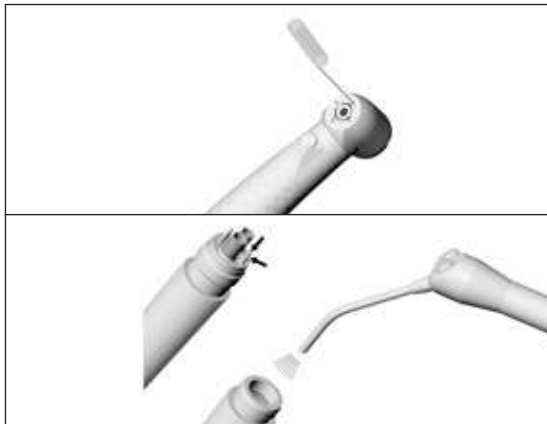

Cleaning of the spray nozzles

- > Clean coolant outlets carefully with the nozzle cleaner to remove dirt and deposits




The nozzle cleaner can be cleaned in an ultrasonic bath and/or in the washer-disinfector

Cleaning of the coolant tubes

- > Blow through the coolant tube using compressed air.



In case of blocked coolant outlets or coolant tubes contact an authorized W&H service partner.

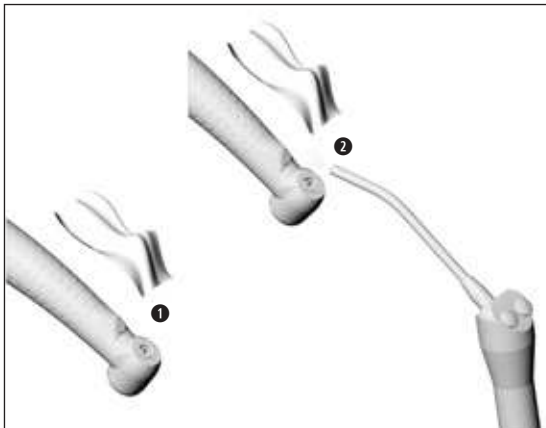

Cleaning of the optic outlet




Avoid scratching of the optic outlet!

- ① Wash the optic outlet with cleaning fluid and a soft cloth.
- ② Blow the optic outlet dry using compressed air or dry it carefully with a soft cloth.




- > Carry out a visual inspection after each cleaning process.
- > Do not use the medical device if the optic outlet is damaged and contact an authorized W&H service partner.

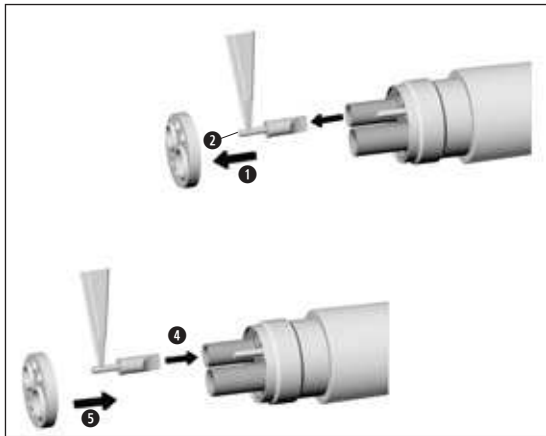

Changing the water filter (RM)

- ➊ Remove the seal.
- ➋ Pull out the water filter with tweezers.
- ➌ Clean the water filter (see page 31).
- ➍ Insert the water filter.
- ➎ Slide on the seal.

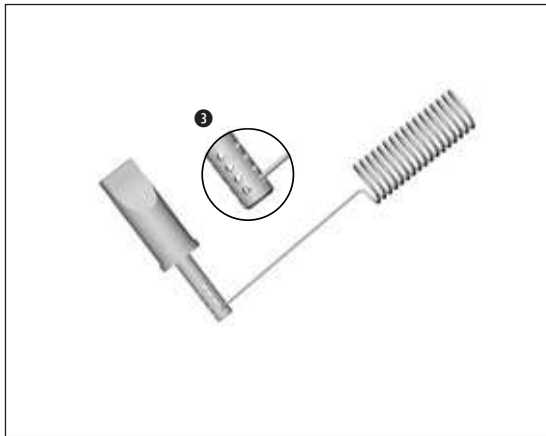

Clean the water filter (RM)

- 3 Use the nozzle cleaner carefully to remove dirt and deposits from the water filter outlets.



The water filter can be cleaned in an ultrasonic bath.



- > Perform a test run.
- > Repeat the complete hygiene and maintenance process.



- W&H recommends automated cleaning and lubrication with W&H Assistina 3x3.
- > Follow the instructions in the Assistina Instructions for use.



> W&H recommends wiping down with disinfectant.



Evidence of the medical device's basic suitability for effective manual disinfection was provided by an independent test laboratory using the »mikrozid[®] AF wipes« disinfectant (Schülke & Mayr GmbH, Norderstedt).



W&H recommends automated cleaning and disinfection using a washer-disinfector (WD).

- > Read the notes, follow the instructions and heed the warnings provided by the manufacturers of washer-disinfectors, cleaning agents and/or disinfectants.



Evidence of the medical device's basic suitability for effective automated disinfection was provided by an independent test laboratory using the >Belimes WD 100< (Firma Belimed AG) washer-disinfector and the >deconex 24 LIQ< cleaning agent (Fa. Borer Chemie) and neutralizer >deconex 26 plus< (Fa. Bohrer Chemie).

- > Cleaning at 65 °C (149 °F) – 5 minutes
- > Disinfection at 90 °C (194 °F) – 5 minutes



- > Ensure that the medical device is completely dry internally and externally after cleaning and disinfection.
- > Remove any liquid residues using compressed air.

Inspection



- > Check the medical device after cleaning and disinfection for damage, visible residual soiling and surface changes.
- > Reprocess any medical devices that are still soiled.
- > Sterilize the medical device following cleaning, disinfection and lubrication.

Lubrication



- > Lubricate the dry medical device immediately after cleaning and/or disinfection.
- > Direct the medical device downwards

Recommended lubrication cycles

- > Essential after every internal cleaning
 - > Essential after every internal cleaning
- or
- > After 30 minutes of use or at least once daily
 - > Chucking system once a week

With W&H Service Oil F1, MD-400

- > Follow the instructions on the oil spray can and on the packaging.

or

With W&H Assistina

- > Follow the instructions in the Assistina Instructions for use.



Lubrication of the chucking system

With W&H Service Oil F1, MD-400

- > Fit the spray adaptor REF 02036100 onto the spray can.
- > Hold the medical device firmly.
- > Press the tip of the spray adaptor firmly into the chucking system
- > Spray for approx. 1 second.

or

With W&H Assistina TWIN / Assistina 301 plus

- > Follow the instructions in the Assistina Instructions for use.

Testing after lubrication



- > Direct the medical device downwards.
- > Operate the medical device so that excess oil can escape.
- > Remove excess oil.



Pack the medical device and the accessories in sterilization packages that meet the following requirements:

- > The sterilization package must meet the applicable standards in respect of quality and use and must be suitable for the sterilization method.
- > The sterilization package must be large enough for the sterilization goods.
- > The filled sterilization package must not be under tension.



W&H recommends sterilization according to EN 13060, EN 285 oder ANSI/AAMI ST79.



- > Read the notes, follow the instructions and heed the warnings provided by the manufacturers of steam sterilizers.
- > The program selected must be suitable for the medical device.

Recommended sterilization procedures

- > Fractionated pre-vacuum process (type B)
- > Gravity displacement process (type N)
- > Sterilization time at least 30 minutes at 121 °C (250 °F) or at least 3 minutes at 134 °C (273 °F)
- > Maximum sterilization temperature 135 °C (275 °F)



Evidence of the medical device's basic suitability for effective sterilization was provided by an independent test laboratory using the LISA 522* steam sterilizer (Firma W&H Sterilization S.r.l., Brusaporto (BG)) and the Siroclav S3** gravitation sterilizer (Sirona).

- > Fractionated pre-vacuum process (type B): temperature 134°C (273 °F) – 3 minutes*
- > Gravity displacement process (type N): temperature 121 °C (250 °F) – 30 minutes**

* according to EN 13060, EN 285, ISO 17665 / ** according to ANSI/AAMI ST55 , ANSI/AAMI ST79



- > Store sterile goods dust-free and dry.
- > The shelf life of the sterile goods depends on the storage conditions and type of packaging.

6. Servicing

Repairs and returns

In the event of operating malfunctions immediately contact an authorized W&H service partner.

Repairs and maintenance work must only be undertaken by an authorized W&H service partner.



- > Ensure that the medical device has been completely processed before returning it.

7. W&H Accessories and spare parts



Use only original W&H accessories and spare parts or accessories approved by W&H.

Suppliers: W&H partners


000301xx	W&H Assistina301 plus
19922000	W&H Assistina 3x2 (MB-200)
19923000	W&H Assistina 3x3 (MB-300)
30310000	W&H Assistina TWIN (MB-302)
02690400	Assistina adaptor for all W&H products with Roto Quick system
02693000	Assistina adaptor for chucking system
10940021	W&H Service Oil F1, MD-400 (6 pcs)
02036100	Spray adaptor for chucking system
02229200	Spray adaptor for all W&H products with Roto Quick system
04396100	<i>Spray adaptor for Multiflex®* connection</i>
05773300	<i>Spray adaptor for NSK Mach®* connection</i>
06024600	<i>Spray adaptor for für Midwest®* connection</i>
02015101	Nozzle cleaner

8. Technical data

Synea Fusion with / without light		TG-98 L / TG-97 L TG-98 L RM / TG-97 L RM	TG-98 LM / TG-97 LM	TG-98 / TG-97 TG-98 L N / TG-97 L N
Coupling according to standard	EN ISO 9168:2009	W&H Roto Quick	Multiflex ^{®*}	W&H Roto Quick / NSK Mach ^{®*}
Rotary instruments	ISO 1797 (∅ mm)	1.6 – 0,01*	1.6 – 0.01	1.6 – 0.01
Max. Length approved by W&H	(mm)	25** / 21**	25** / 21**	25** / 21**
Minimum chucking length		until back stop	until back stop	until back stop
Max. operating part diameter	(mm)	2	2	2
Idle mode speed (± 30,000)	(min ⁻¹)	360,000 / 390,000	360,000 / 390,000	360,000 / 390,000
Coolant supply volume	ISO 14457 (ml/min)	> 50	> 50	> 50
Water setting range (Recommended water pressure)	(bar)	0.7 – 2 (1.5)***	0.7 – 2 (1.5)***	0.7 – 2 (1.5)***
Chip air setting range (Recommended chip air pressure)	(bar)	1.5 – 3 (2)***	1.5 – 3 (2)***	1.5 – 3 (2)***
Exhaust air pressure	(bar)	< 0.5	< 0.5	< 0.5
Operating pressure	(bar)	3 ± 0.3	2.5 – 4	3 ± 0.3
Recommended operating pressure	(bar)	–	3 + 0.2	–
Air consumption	(Nl/min)	45	45	45
Supply voltage Roto Quick connection nominal	(V DC oder V AC)	3.2	–	–
Supply voltage range	V AC	2.2 – 4.2	–	–
Supply voltage range	V DC	2.2 – 6	–	–
Current consumption	(A)	0.2	–	–
Chip air consumption at 2 bar	[Nl/min]	> 1.5	> 1.5	> 1.5

* see page 47

* *Multiflex® and NSK Mach® are trademarks of third parties not affiliated with W&H Dentalwerk Bürmoos GmbH.*

 ** When using longer rotary instruments the user must ensure by correct selection of the operating conditions, that there is no danger to the user, patient or third parties.

*** Chip air pressure / water pressure must be set at the same time
Chip air pressure / water pressure must be set at the same time

Power and speed data of turbine handpieces are largely dependent on the quality of the turbine hoses used and may therefore differ from the specified values.

$\text{rpm} = \text{min}^{-1}$ (Revolutions per minute)

Temperature information



Temperature of the medical device on the operator side: maximum 55 °C (131 °F)

Temperature of the medical device on the patient side: maximum 50 °C (122 °F)

Temperature of the working part (rotary instrument): maximum 41 °C (105.8 °F)

Ambient conditions

Temperature during storage and transport:

-40 °C to +70 °C (-40 °F to +158 °F)

Humidity during storage and transport:

8 % to 80 % (relativ), non-condensing

Temperature during operation:

+10 °C to +35 °C (+50 °F to +95 °F)

Humidity during operation:

15 % to 80 % (relativ), non-condensing

9. Disposal



Ensure that the parts are not contaminated on disposal.

Instrument disposal



Follow your local and national laws, directives, standards and guidelines for disposal.

- > Medical device
- > Waste electrical equipment
- > Packaging

Explanation of warranty terms

This medical device has been manufactured with great care by highly qualified specialists. A wide variety of tests and controls guarantee faultless operation. Please note that claims under warranty can only be validated when all the directions in the Instructions for use have been followed.

As manufacturer, W&H is liable for material or manufacturing defects within a warranty period of 12 months from the date of purchase.

We accept no responsibility for damage caused by incorrect handling or by repairs carried out by third parties not authorized to do so by W&H!

Claims under warranty accompanied by proof of purchase, must be sent to the vendor or to an authorized W&H service partner. The provision of service under warranty extends neither the warranty period nor any other guarantee period.

12 months warranty

Authorized W&H service partner

Find you nearest W&H service partner at <http://wh.com>

Simply go to the menu option »Service« for full details. Alternatively please contact:

W&H (UK) Limited, Unit 6, Stroud Wood Business Centre, Park Street, St Albans, AL2 2NJ Hertfordshire
t + 44 1727874990, f + 44 1727872254, E-Mail: technical.uk@wh.com

W&H IMPEX INC., 6490 Hawthorne Drive, Windsor, Ontario, N8T 1J9, Canada
t + 1 519 9446739, f + 1 519 9746121, E-Mail: service.ca@wh.com

W&H IMPEX INC., 33091 W Jefferson Ave., Brownstown, MI-48173, USA
t + 1 800 265 6277, +1 519 944 6739, f +1 519 974 6121, E-Mail: service.us@wh.com

W&H Austria GmbH, Ignaz-Glaser-Straße 53, 5111 Bürmoos, Austria
t +43 6274 6236-239, f +43 6274 6236-890, E-Mail: office.at@wh.com

A-DEC AUSTRALIA CO. INC., Unit 8, 5-9 Ricketty Street, Mascot NWS 2020, Australia
t + 61 2 83324000, f + 61 2 83324099, E-Mail: a-dec@a-dec.com.auw

Manufacturer

W&H Dentalwerk Bürmoos GmbH
Ignaz-Glaser-Straße 53, 5111 Bürmoos, Austria

t +43 6274 6236-0, f +43 6274 6236-55
office@wh.com wh.com

Form-Nr. 50743 AEN
Rev. 006 /19.04.2019
Subject to alterations